

Certificate of Analysis

BPC-157 · 10 mg per vial · batch VX351222

SUBMITTED BY Anonymous submitter	SAMPLE RECEIVED 4 August 2026	REPORT ISSUED 25 August 2026
COMPOUND BPC-157	DECLARED CONTENT 10 mg per vial	TESTS ORDERED Full panel

Results

PARAMETER	RESULT	SPECIFICATION	
Identity HPLC, retention time against reference standard	Matches reference	Matches reference	CONFORMS
Purity HPLC-DAD, 214 nm, area %	99.31%	≥ 98.0%	CONFORMS
Content HPLC-DAD against reference	10.04 mg / vial	90 to 110% of label	CONFORMS
Endotoxin LAL, kinetic chromogenic	2.1 EU / vial	≤ 5.0 EU / vial	CONFORMS
Aerobic count and yeast/mould TAMC / TYMC	< 10 CFU / vial	TAMC ≤ 100, TYMC ≤ 10 CFU / vial	CONFORMS
Escherichia coli Presumptive presence	Not detected	Not detected	CONFORMS
Salmonella spp. Presence	Not detected	Not detected	CONFORMS

All parameters tested conform to the stated specification.




Verify this report

Scan the code, or enter VT-7K2M9QF at veritalys.com/verify. The record shown there is the one this document was generated from. If any field differs, this document has been altered.
Lookups are free, need no account, and show the same record to everyone who holds the number.

Analysis performed by an independent partner laboratory in the European Union. Report issued and verified by Veritalys. Veritalys does not perform analysis itself.
For research and quality verification only. Not medical advice. This report does not make any product safe or lawful for human use.

Figure 1 Chromatogram

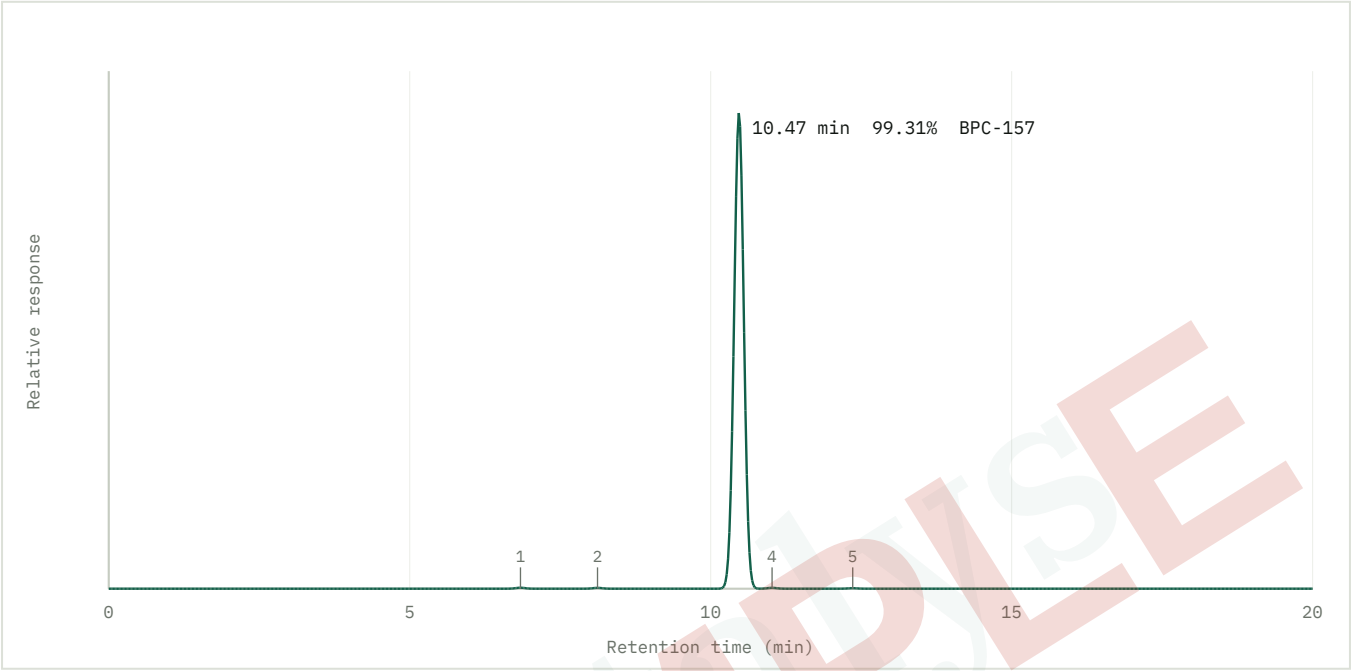

PEAK	RETENTION TIME (MIN)	AREA %	NAME
1	6.84	0.21	
2	8.12	0.18	
3	10.47	99.31	BPC-157
4	11.02	0.19	
5	12.36	0.11	

Drawn from the peak table reported by the laboratory: each peak is placed at its measured retention time and sized to its measured share of total peak area. Peak widths are schematic.

How to read this report

Identity	Whether the vial holds the compound it claims to. Your sample is run next to a known-pure reference standard of that compound, and the two have to match.
Content	How many milligrams of peptide are actually in the vial, measured against the reference standard. This is the number that catches under-filled vials.
Purity	The main peak's share of everything the detector saw. It is a ratio, not a quantity, which is why it is reported next to content rather than instead of it.
Endotoxin	Bacterial debris that survives sterilisation, reported as a quantity in endotoxin units (EU), not as the word negative.
Microbiology	Total aerobic count, yeast and mould, E. coli and Salmonella. The cultures need several days to grow, which is why panels that include them take longer.
Specification	The acceptance limit each result is judged against. Conforms means the result sits inside it.

What this report covers

One vial: the one received on 4 August 2026, carrying batch VX351222. It says nothing about any other vial or any other batch, and the tested unit is consumed by the analysis. Confidence in a batch comes from testing each batch.

The name under Submitted by is whatever the customer typed when ordering. Left blank, it reads Anonymous submitter. Veritalys publishes no directory of results. A report is reachable only by its own number, and who receives that number is the customer's decision.